




K-1215




K-1515

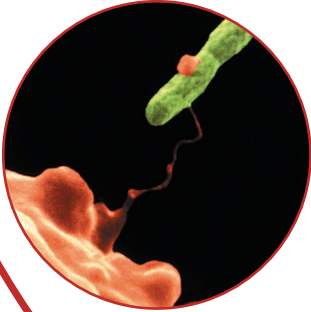

Legionella K-Set


Rapid diagnostic test for *in vitro* detection of *Legionella pneumophila* LPS antigen in urine samples

- One Step!
No dilution required!
- Easy to read
- Specific and sensitive
- Safe
- One of the best Legionella kit on the market!

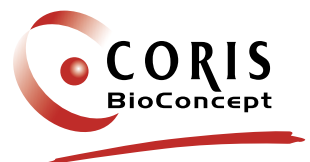

www.corisbio.com

Legionella K-SeT

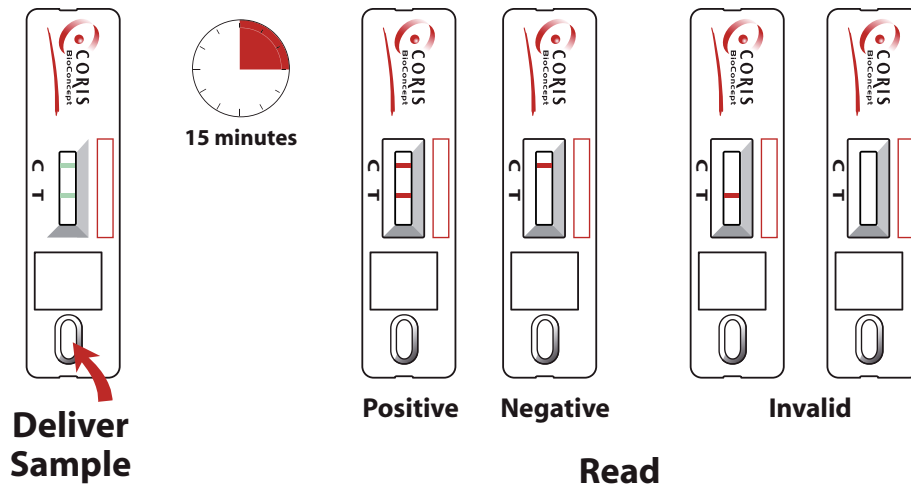

Performance of the kit

	Compared to EIA (n=109)	
Sensitivity	90.0%	(73.3 to 97.4%)
Specificity	100%	(91.9 to 100%)
PPV	100%	(84.5 to 100%)
NPV	94.8%	(84.7 to 98.7%)
Agreement	96.5%	(82/85)

For more technical information

client.care@corisbio.com

Ordering Information

PRODUCT NAME	DESCRIPTION	STORAGE	CODE
Legionella K-SeT	20 cassettes, 20 transfer pipettes	4°C to 30°C	K-1215
Legionella K-SeT with controls	20 cassettes, 20 transfer pipettes, positive and negative controls	4°C to 30°C	K-1515

— Distributed by —



CREALYS Science Park
Rue Guillaume Fouquet 11
5032 Gembloux - BELGIUM
T +32 (0)81 719 910 - F +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com



MADE IN BELGIUM

D-CUS-10-15-K/04
March 2023